

Moisture meter

Operating Manual humimeter BLL


Moisture meter with insertion probe for the determination of the moisture content of wood chips



8,0°F | 6,16%| 456kg/m³| -27,3td|0,64aw|51,9%r.H.|14,8%abs|100,4g/m²|09m/s|4,90Ugl|

Your humimeter BLL at a glance

The whole unit

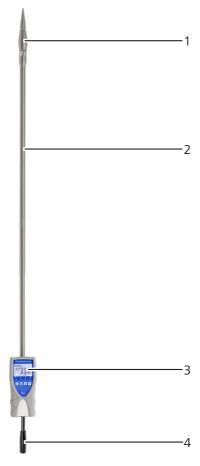

No	Name
1	Measuring head
2	Insertion probe
3	Electronics in plastic housing
4	Handle bar



The main unit



No	Name
1	USB port (optional)
2	Display
3	Keypad
4	Rubber protection cover

Rear of the main unit



No	Name
1	Battery compartment

The display



No	Name
1	Calibration curve
2	Moisture content % ("6.1 How moisture content is defined")
3	Display symbols
4	Temperature display

The display symbols

Symbol	Name
4	Enter
	Up
-	Down
4	Back
09	Enter numbers
AZ	Enter letters
]	Continue / go right
	Left
V	Yes

Symbol	Name
X	No
Û	Change input level
OK	ОК
\$.	Change menu
1	Enter data
<u>"Ono"</u>	View measurements
Ä	Delete measurements
\odot	On/off button, display light
	Save measured value



The menus

The device has four different menus: Data Log, product selection, additional function and main menu:

Data Log menu



No	Name
1	Change menu
2	Display illumination / device on/off
3	Save measured value
4	Show the last recorded values

Product selection menu



No	Name
1	Change menu
2	Display illumination / device on/off
3	For changing the calibration curve

Additional function menu



No	Name
1	Change menu
2	Display illumination / device on/off
3	Mirror display

Main menu

The main menu comprises the following menu items:

- Edit Logs:
 - Manual Logs, Clear Logs
- Print Logs:

Last Log, All Logs, Clear Logs

- Send Logs:
 - Manual Logs, Clear Logs
- · Options:

Bluetooth, Date/Time, Log Time, Language, Unlock, °C/°F, BL On Time, Auto Off Time, Materialcalib., Password, Reset

Status



Table of contents

Your	numimeter BLL at a giance	∠
The wh	nole unit	2
The ma	ain unit	3
Rear of	the main unit	3
The dis	play	4
The dis	play symbols	4
The me	enus	5
1.	Introduction	10
1.1	Information about this operating manual	10
1.2	Limitation of liability	10
1.3	Symbols used in this manual	11
1.4	Customer service	11
2.	For your safety	12
2.1	Proper use	12
2.2	Improper use	12
2.3	User qualifications	12
2.4	General safety information	13
2.5	Waranty	13
3.	On receipt of your device	13
3.1	Taking the device out of its packaging	13
3.2	Making sure that all of the components have been included	14
3.3	Inserting batteries	15
4.	Using the device - Basics	16
4.1	Switching the device on	16
4.2	Selecting the calibration curve	16
4.3	Taking a measurement	16
4.4	Mirroring the dispay	17
4.5	Switching the device off	17
5 .	The measuring process	17
5.1	Preparing a measurement	17

5.2	Taking a measurement	18
5.3	Hold function - Freezing the displayed values	19
5.3.1	Activating the Hold function in the Options menu	19
5.3.2	Using the Hold function	19
5.4	Saving individual readings	20
5.4.1	Activating the manual save function in the options menu	20
5.4.2	Using the manual save option	20
5.5	Saving several readings (a measurement series) at the same time	21
5.6	Viewing individual readings	23
5.7	Viewing individual readings from a series of measurements	23
5.8	Deleting all measured values (data log)	24
5.9	Deleting individual measurement series	24
5.10	Deleting individual values from a single series of measurements	25
6.	Calibration curves	26
6.1	How moisture content is defined	26
6.2	Definition wood chip types (in accordance with EN ISO 17225-1)	26
6.3	Selection of calibration curve for wood chips	
6.3.1	Wood chips	27
6.3.2	Coarse wood chips	27
6.3.3	Industrial wood chips	27
6.4	Notes for comparative measurement with oven-drying method	31
6.5	Compression of wood chips	31
7.	Using the LogMemorizer program	32
7.1	Installing / opening the program	32
7.2	Exporting measured values to a computer	33
8.	Checking on the device's status	35
9.	Configuring the device	36
9.1	Turning on Bluetooth	36
9.2	Adjust the date/time	36
9.3	Selecting a language	37
9.4	Activating options	37
9.5	Deactivating options	38



9.6	Selecting °C/°F	38
9.7	Reducing the device's power consumption	38
9.7.1	Configuring the display illumination time	38
9.7.2	Configuring automatic switch-off	39
9.8	Configuring the material calibration function	40
9.9	Changing the password	40
9.10	Resetting the device to its factory settings	41
10.	Cleaning and maintenance	41
10.1	Changing batteries	41
10.2	Cleaning the device	42
11.	Accessories	43
11.1	BLL tube extension	43
11.1.1	Overview tube extension and humimeter BLL	43
11.1.2	Demounting of the measuring tip	44
11.1.3	Installation of the extension	44
11.1.4	Tip assembly	45
11.1.5	Function test	45
11.2	Changing the measuring head (tip)	45
12.	Faults	46
13.	Storage and disposal	47
13.1	Storing the device	47
13.2	Disposing of the device	47
14.	Device information	48
14.1	CE declaration of conformity	48
14.2	Technical data	52
15.	Notes	53

1. Introduction

1.1 Information about this operating manual

This operating manual is designed to enable you to use the humimeter BLL safely and effectively. It is part of the device, has to be stored nearby and must be easily accessible to users at all times.

All users are required to carefully read and make sure that they have understood this operating manual before using the humimeter BLL. All of the safety and operating instructions detailed in this manual have to be observed to ensure the safety of the device.

1.2 Limitation of liability

All of the information and instructions provided in this operating manual have been compiled on the basis of the current standards and regulations, the state of the art, and the extensive expertise and experience of Schaller Messtechnik GmbH.

Schaller Messtechnik GmbH does not accept any liability for damage associated with the following, which also voids the warranty:

- Non-observance of this operating manual
- Improper use
- Inadequately qualified users
- · Unauthorised modifications
- Technical changes
- Use of unapproved spare parts

This fast measuring procedure can be affected by a range of different factors. For this reason, we recommend periodically checking the device's measurements with a standardised oven-drying method.

We, as the manufacturer, do not accept any liability for any incorrect measurements and associated consequential damage.



1.3 Symbols used in this manual

All of the safety information provided in this manual is shown with a corresponding symbol.



CAUTION

It is essential to observe this warning. Non-compliance can lead to injury.



ATTENTION

It is essential to observe this warning. Non-compliance can lead to damage to property or equipment.



Information

This symbol indicates important information that enables users to use the device more efficiently and cost-effectively.

1.4 Customer service

For technical advice, please contact our customer service department at:

Schaller Messtechnik GmbH Max-Schaller-Straße 99 A - 8181 St.Ruprecht an der Raab

Telefon: +43 (0)3178 28899 Fax: +43 (0)3178 28899 - 901

E-Mail: info@humimeter.com Internet: www.humimeter.com

© Schaller Messtechnik GmbH 2024



2. For your safety

The device complies with the following European directives:

- Restriction of Hazardous Substances in Electrical and Electronic Equipment (RoHS)
- Electromagnetic compatibility (EMC)

The device corresponds to state-of-the-art technology. However, it is still associated with a number of residual hazards.

These hazards can be avoided through strict observance of our safety information.

2.1 Proper use

- Easy to use device for guickly measuring the moisture content of wood chips
- The device must only be used for taking measurements on the products defined in the following sections of this manual (see "6. Calibration curves").

2.2 Improper use

- The device must not be used in ATEX.
- The device is not suitable for measuring frozen wood chips or wood chips with a temperature over +40 °C.
- The device is not waterproof and must be protected from water and fine dust (IP40).

2.3 User qualifications

The device must only be operated by people who can be expected to reliably take the measurements. The device must not be operated by people whose reaction times may be slowed due to, e.g. the use of drugs, alcohol or medication.

All persons using this device must have read, understood and follow the instructions provided in the operating manual.



2.4 General safety information

The following safety information has to be observed at all times to avoid damage to objects and injury to people:

- Remove the batteries if the device isn't used for a prolonged period of time.
- Keep the measuring head away from your body throughout all activities.
- Keep the measuring head away from other people throughout all activities.
- In case of damages or loose parts on the device, remove the batteries and contact Schaller Messtechnik GmbH or your dealer.

All of the device's technical features have been inspected and tested before delivery. Every device has a serial number. Do not remove the tag with the serial number.

2.5 Waranty

The warranty does not apply to:

- Damage resulting from non-observance of the operating manual
- Damage resulting from third-party interventions
- Products that have been used improperly or modified without authorisation
- Products with missing or damaged warranty seals
- Damage resulting from force majeure, natural disasters, etc.
- Damage from improper cleaning
- Batteries older than six months
- Damage resulting from improper strain (pressure, bending) of the insertion probe or the measuring head
- Damage by dropping the measuring head

3. On receipt of your device

3.1 Taking the device out of its packaging

- Take the device out of its packaging.
- Next, make sure that it is not damaged and that no parts are missing.

3.2 Making sure that all of the components have been included

Make sure that all of the components have been included by checking the package contents against the following list:

- humimeter BLL
- 4 pieces of AA Alkaline batteries
- Rubber protection cover
- Handle bar
- · Operating manual

Optional accessories:

- humimeter USB data interface module USB flash drive with software and USBcable or download using humimeter.com/software
- Battery-powered portable thermo printer (can only be used in combination with humimeter USB data interface module) - described in a separate user manual.
- Bluetooth module (can only be used in combination with humimeter USB data interface module) - described in a separate user manual.
- Wooden case
- · Replacement measuring head
- 1 meter tube extension
- Test block




3.3 Inserting batteries


 Remove the rubber protection cover. To do so, hold the rubber protection cover at the upper side and pull it over. If your device is provided with an optional USB port, remove the protection cap of the USB socket before (figure 1 and 2).









3. Take hold of the device with one hand, press your thumb onto the engraved area of the battery compartment (1) and drag downwards (2) (figure 4).















4. Using the device - Basics

4.1 Switching the device on

- Press the button for 3 seconds.
- » The display will then show the status indicator (figure 7).
- » After inserting the batteries, the device switches on automatically.



4.2 Selecting the calibration curve

To do so: The device has to be in the product selection menu (figure 8).

For an overview of the different calibration curves and the criteria for selecting them, please refer to "6. Calibration curves".

- 1. Press the ♥ or ♠ button to move from one product to the next Or
- 2. Press the or button for 3 seconds to open the calibration curve overview (figure 9).
- Use the arrow keys to move from one calibration curve to the next
- 4. and keep any of them pressed to scroll through the types.
- 5. Confirm your selection by pressing 📲.
 - » The calibration curve you selected will now be shown at the top of the display.

4.3 Taking a measurement

 For information on how to take a measurement, see section "5. The measuring process".







4.4 Mirroring the dispay

To do so: The device has to be in the additional function menu (figure 10).

- Press the button to mirror the display.
- Press the button again to cancel the mirroring of the display.



4.5 Switching the device off

To do so: The device has to be in the product selection, the Data Log or the additional function menu. It is not possible to switch off the device when it is in the main menu.

• Press the 🖒 button for 3 seconds.

5. The measuring process

5.1 Preparing a measurement

To do so: The device has to have nearly the same temperature than the product being measured. It is recommended to let your humimeter device adjust to the surrounding temperature of the wood chips before the measurement.

- Switch on the device (see "4.1 Switching the device on").
- Select the desired calibration curve (see "6. Calibration curves") by pressing the or button (see "4.2 Selecting the calibration curve"rve") (figure 12).





5.2 Taking a measurement

To do so: The device has to have nearly the same temperature than the product being measured.

- Insert the measuring head of the device straight into the wood chips (figure 13).
- » Do not bend or drop the measuring head!
- The device will now instantly display the moisture content on the display (figure 14).
- » The displayed value flashes when the moisture content exceeds 40 % (figure 15). A flashing value signals lowered accuracy of the measurement. The device has a measuring range of 10 % to 50 % water content.
- » Once the reading has been taken, it can be saved on the device (see "5.4 Saving individual readings" or "5.5 Saving several readings (a measurement series) at the same time").









CAUTION

Risk of injury

Risk of injury due to the measuring head

- ► Keep the measuring head away from your body throughout all activities.
- ► Keep the measuring head away from other people throughout all activities.

Information - Measuring accuracy

This rapid and non-destructive measuring procedure allows you to quickly take moisture readings at a number of different points. When saving the individual readings, the device will automatically calculate the readings' average (see "5.5 Saving several readings (a measurement series) at the same time").



Information - Incorrect readings

Always make sure to select the correct calibration curve for the material you are measuring. This prevents taking incorrect readings (see "11. Accessories").



5.3 Hold function - Freezing the displayed values


The device can be configured in such a way that the information being shown on the display will freeze at the touch of a button until a new button is pressed. This function can be very useful when e.g. taking readings in spaces where it is not possible to see the display (e.g. overhead).

5.3.1 Activating the Hold function in the Options menu

To do so: The device has to be switched on and be in the product selection menu.


- 1. Press three times or hold for 2 seconds.
- 2. Select **Options**. To do so, press **T** or **a** and confirm by pressing **4**.
- 3. Select **Log Time** (figure 16). To do so, press **r** or **and confirm by pressing**.





- 5. Press to leave the **Options** menu.
- 6. Press **t** to leave the main menu.





5.3.2 Using the Hold function

To do so: The device has to be switched on and be in the Data Log menu (see "Data Log menu" page 5).

- » The current reading will be frozen. All of the four symbols will now be displayed as [1] (figure 18).
- To reactivate the frozen display, simply press any button.



5.4 Saving individual readings

The device can be configured in such a way that the device will save a reading every time a button is pressed. This option (manual save function) is the device's default setting.

5.4.1 Activating the manual save function in the options menu

To do so: The device has to be switched on and be in the product selection menu.


- 1. Press three times or hold for 2 seconds.
- 2. Select **Options**. To do so, press **T** or **A** and confirm by pressing **4**.
- 3. Select **Log Time** (figure 19). To do so, press **T** or **and confirm by pressing 4**.
- 4. Select **Manual** (figure 20). To do so, press or and confirm by pressing .
 - The setting has been saved.
- 5. Press 👫 to leave the **Options** menu.
- 6. Press to leave the main menu.

5.4.2 Using the manual save option

To do so: The device has to be in the Data Log menu (see "Data Log menu" page 5). The manual save option is set on the device.


- 1. Press
 - » The display will now appear as shown in figure 22 and the disc symbol will be preceded by the digit one
- 2. Press to enter a name for the saved reading and to finish the measuring process.
 - » The display will now appear as shown in figure 23.













3. The data you have inputted can be overwritten at any time.

4. Inputting letters:

Press and hold [4] ... Z to quickly scroll to the required letter and either press it for 3 seconds or press [4] to confirm the selected letter (figure 24).



5. Inputting numbers:

Press and hold **11...** to quickly scroll to the required number and either press it for 3 seconds or press **4...** to confirm the selected number.

6. Moving forward/back:

Press to switch to another input level. Press or to move forward or back.

- 7. Confirm your entry by pressing 🚚.
 - » The data you entered has been saved.

5.5 Saving several readings (a measurement series) at the same time

To do so: The device has to be in the Data Log menu (see "Data Log menu" page 5).

- 1. Take several readings of the same wood chips (see "5. The measuring process").
- 2. To save a reading, press as soon as the reading has been taken.



- » The display will now appear as shown in figure 25. The marked number shows the number of readings that have already been saved.
 26
 26.5%
 24.5
 24.5
- Press to enter a name for the saved series of measurements and to finish the measuring process.



- » The display will now appear as shown in figure 26.
- 4. The data you have inputted can be overwritten at any time.

5. Inputting letters:

Press and hold [4] ... To quickly scroll to the required letter and either press it for 3 seconds or press [4] to confirm the selected letter (figure 27).




6. Inputting numbers:

Press and hold ... • to quickly scroll to the required number and either press it for 3 seconds or press to confirm the selected number.

7. Moving forward/back:

Press to switch to another input level. Press to move forward or back.

- 8. Confirm your entry by pressing 🚚.
 - » The data you entered has been saved.
 - » The device automatically determines the average moisture content of the saved measuring values.
 - » The display will show the following information:



No	Name
1	Name of the measurement series (editable)
2	Temperature (average)
3	Date & start time of the measurement series
4	Date & end time of the measurement series
5	Number of saved readings
6	Calibration curve
7	Device name
8	Moisture content (average)




5.6 Viewing individual readings

To do so: You must have saved a reading (e.g. 1 log) The display will now appear as shown in figure 28.

- 1. Press 'm'.
- - » The display will now appear as shown in figure 29.
 - » Press 👫 to leave this screen.






5.7 Viewing individual readings from a series of measurements


To do so: You must have saved a series of measurements (e.g. 2 logs).

The display will now appear as shown in figure 30.

- 1. Press 'oro'.
- 2. Navigate to the required measurement series. To do so, press or ...
 - » The display will now appear as shown in figure 31.
- 3. Press to switch to another input level.
 - » The display will now appear as shown in figure 32.
- 4. Press 'cro' again.
 - » The display will now appear as shown in figure 33.
- Navigate to the required reading (No.: 1, No.: 2, No.: 3). To do so, press or or or .
- 6. Press | to leave this screen.











5.8 Deleting all measured values (data log)

To do so: You must have taken and saved one or several readings.

- 1. Press \$\frac{1}{4}\$ three times or hold for 2 seconds.
- Select Edit Logs (figure 34). To do so, press ▼ or
 and confirm by pressing ➡.
- 3. Select **Clear Logs** (figure 35). To do so, press **T** or **a** and confirm by pressing **4**.
 - » The display will show the message clear? (figure 36).
- 4. Confirm by pressing **v**.
 - » The data log has been deleted.
- 5. Press 👫 to leave the **Edit Logs** menu.
- 6. Press 🔓 to leave the main menu.








5.9 Deleting individual measurement series

To do so: You must have saved a measured value (e.g. **1** log) or a series of measurements (e.g. **3** logs). The display will now appear as shown in figure 37.

- 1. Press '0-0'.
 - » The display will now appear as shown in figure 38.
- 2. Select the required reading. To do so, press T or
- 3. Press 😱 to switch to another input level.
 - The display will now appear as shown in figure 39.
- 4. Press 🧵.









- » The display will then show the message clear? (figure 40).
- 5. Confirm by pressing 🎺.
 - » The value has been deleted.




5.10 Deleting individual values from a single series of measurements

To do so: You must have saved a series of measurements comprising at least 2 logs. The display will now appear as shown in figure 41.


- 1. Press 'cro'.
 - » The display will now appear as shown in figure 42.
- 2. Select the required reading. To do so, press T or
- 3. Press to switch to another input level.
 - The display will now appear as shown in figure 43.
- 4. Press '000'.
 - » The display will now appear as shown in figure 44.
- 6. Press **\(\rightarrow\)** to switch to another input level.
 - » The display will now appear as shown in figure 45.
- 7. Press I to delete the value shown.
 - » The display will then show the message clear? (figure 46).
- 8. Confirm by pressing 📢.
 - » The value has been deleted.














6. Calibration curves

Calibration curve	Wood chip type	Measuring range
Wood chips	See "6.3.1 Wood chips"	10 % - 50 %
Coarse wood chips	See "6.3.2 Coarse wood chips"	10 % - 50 %
Industrial wood chips	See "6.3.3 Industrial wood chips"	10 % - 50 %
Test block	! Only for testing the moisture meter !	

6.1 How moisture content is defined

The device measures and shows a material's moisture content. The moisture content readings it displays are calculated in relation to the material's overall mass:

$$\%WG = \frac{M_n - M_t}{M_n} \times 100$$

M_n: Mass of the sample with average moisture content

M_t: Mass of the sample with zero moisture content

%WG: Moisture content (in accordance with EN ISO 18134-2)

6.2 Definition wood chip types (in accordance with EN ISO 17225-1)

The given numbers refer to the particle sizes that fit through the round screen openings.

P16 at least 75 % of the mass between 3.15 and 16 mm

• P31 at least 75 % of the mass between 8 and 31.5 mm

• P45 at least 75 % of the mass between 8 and 45 mm

P63 at least 75 % of the mass between 8 and 63 mm



6.3 Selection of calibration curve for wood chips

The calibration curves for wood chips depend on the wood type (hardwood, softwood), the size of the chips (size classes according to norm EN ISO 17225-1) as well as on the content of fine fraction.

If you are not sure which calibration curve is the best suited for your material, it is recommended to carry out a reference measurement by kiln-drying (according to EN ISO 18134-2).

Schaller Messtechnik GmbH will be happy to advise you on the selection of the right calibration curve. Please send a picture of your wood chips, placing a measuring tape to the material, to support@schaller-gmbh.at. You will receive a recommendation from us immediately.

6.3.1 Wood chips

For wood chips with fine fraction, mainly consisting of hardwood (maximum proportion of softwood of 30 %). For wood chips sizes from P31 to P45. The fine fraction mainly derives from barks, small branches and bushes. See example pictures 47 and 48.

If your wood chips don't contain small parts (few fine fraction or no fine fraction) or if the wood chips contain a higher proportion of softwood, use one of the following calibration curves.

6.3.2 Coarse wood chips

For coarse wood chips without fine fraction, mainly consisting of hardwood (maximum proportion of softwood of 30 %). This curve also has to be used for wood chips with fine fraction, mainly consisting of softwood, with a proportion of softwood (spruce, fir, pine, larch) of 70 % and more. For wood chips sizes from P31 to P63. See example pictures 49 and 50.

If your wood chips mainly consist of softwood and don't contain small parts (few fine fraction or no fine fraction), use the following calibration curve.

6.3.3 Industrial wood chips

For coarse wood chips without fine fraction, mainly consisting of softwood, with a proportion of softwood (spruce, fir, pine, larch) of 70 % and more. For wood chips sizes from P45 to P63. This curve is predominantly suited for measuring wood chips deriving from logs and full trees as well as sawmill residues without fine fraction. See example pictures 51 and 52.

Example pictures wood chips





Example pictures coarse wood chips





Example pictures industrial wood chips







6.4 Notes for comparative measurement with oven-drying method

The device uses a much higher sample quantity than the drying oven (12-fold to 20-fold quantity of kiln-drying method). Furthermore, to determine a more accurate average moisture value in case of inhomogeneous material, there can be effected several measurements within a short time.

Considering a sampling error due to the considerably smaller sample quantity as well as the content of volatile matters (resin etc.) that are not water, the kiln-drying method will practically reach an accuracy of approx. +/- 3 %. Therefore, if the measuring values of these two very different methods of determining the water content are compared, differences of +/- 3 % can be considered to be normal.

In the standard EN ISO 18134-2 is declared that the drying oven method provides no absolute values, but only comparable values.

6.5 Compression of wood chips


The humimeter BLL is calibrated for normally compressed wood chips. If the wood chips being measured are much less or much more compressed, the accuracy of the measurement will decrease. Normally compressed wood chips are defined in norm EN 15103 (determination of the bulk density).

7. Using the LogMemorizer program

To do so: The device is provided with USB interface, and the USB stick with LogMemorizer software and USB cable are available. Otherwise, you can also install the software at humimeter.com/software or by scanning the QR code.

7.1 Installing / opening the program

- Insert the USB stick with the LogMemorizer program into the USB port on your computer or
 - » download the LogMemorizer software at humimeter.com/software or use the QR code.
- 2. Open the **setup** application.
- 3. Follow the installation instructions.
- 4. Open LogMemorizer.
 - The screen will now display the LogMemorizer's interface (figure 53).

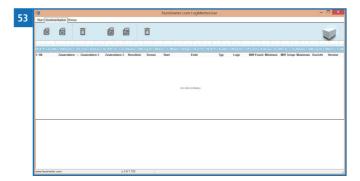

» Before using LogMemorizer, please refer to the the separate LogMemorizer operating manual for the correct configuration of the USB COM Port.

For more information on LogMemorizer, please refer to the separate LogMemorizer operating manual supplied with the device.



7.2 Exporting measured values to a computer

To do so: LogMemorizer must be installed. And you must have taken and saved one or several moisture readings.


Options: You can export moisture readings from the humimeter BLL or initiate the export at your computer.

Exporting moisture readings from the humimeter BLL

Connect the humimeter BLL to your computer using the supplied USB cable:

- 1. Insert the USB Mini B connector into the humi meter BLL (figure 54).
- 2. Insert the USB connector into the computer.
- 3. Open LogMemorizer on your computer.
- 4. Switch on the humimeter BLL.
- 5. Press 4 three times or hold for 2 seconds.
- 6. Select **Send Logs** (figure 55). To do so, press or and confirm by pressing.
- 7. Select **Manual Logs** (figure 56). To do so, press or **A** and confirm by pressing **4**.
 - » The display will then show the message **Send** (figure 57).
 - » All of the measuring values saved on the humimeter BLL will now be sent to your computer.









Initiating the data export at your computer

Connect the humimeter BLL to your computer using the supplied USB cable:

- Insert the USB Mini B connector into the humi meter BLL (figure 58).
- 2. Insert the USB connector into the computer.
- 3. Open LogMemorizer on your computer.



- 4. Switch on the humimeter BLL.
- 5. Open the **Communication** tab in LogMemorizer (figure 59).



- 6. Select and click on one of the two buttons shown in figure 60.
 - » Import all manual logs (for importing all manually saved readings) or
 - » Import most recent manual log (for importing the most recent manually saved logs).



No	Name
1	Import all manual logs
2	Import most recent manual log

» The measuring values saved on the humimeter BLL will now be sent to your computer.



8. Checking on the device's status

- 1. Press Three times or hold for 2 seconds.
- 2. Select **Status**. To do so, press \P or \ddot and confirm by pressing \ddot .
 - » The display will then show the status indicator humimeter.
 - » The display will show the following information:



No	Name
1	Serial number
2	Software version
3	Battery status
4	Memory status

- 3. Confirm by presssing 🟑.
- 4. Press 🔓 to leave the main menu.

9. Configuring the device

9.1 Turning on Bluetooth

The information on Bluetooth is provided in a separate operating manual.

9.2 Adjust the date/time

- 1. Press three times or hold for 2 seconds.
- 2. Select **Options**. To do so, press \P or \red and cofirm by pressing \red .
- 3. Select **Date/Time**. To do so, press **T** or **L** and cofirm by pressing **L**.
 - » The display will now appear as shown in figure 61.
 - » The format for the date is **DD-MM-YY** (Day-Month-Year).
 - » The format for the time is hh:mm:ss (Hour:Minutes:Seconds).
- 4. Inputting numbers:

Press and hold **1 1 1** to quickly scroll to the required number and either press it for 3 seconds or press to confirm the selected number (figure 62).




To move forward between **DD-MM-YY** and **hh:mm:ss**, press **b**.

6. Moving back:

Press to switch to another input level. To move backward between **DD-MM-YY** and **hh:mm:ss**, press ...

- 7. Confirm the date/time by pressing **IK**.
 - » The settings have been saved.
- 8. Press 4 to leave the **Options** menu.
- 9. Press **t** to leave the main menu.





9.3 Selecting a language

- 1. Press three times or hold for 2 seconds.
- 2. Select **Options**. To do so, press \P or \red and cofirm by pressing \red .
- 3. Select Language. To do so, press \P or \red and cofirm by pressing \red .
- 4. Navigate to the required language. To do so, press \P or \dbela and cofirm by pressing \dbela .
 - » The settings have been saved.
- 5. Press 4 to leave the **Options** menu.
- 6. Press to leave the main menu.


9.4 Activating options

To do so: Some of the options must be deactivated.

- 1. Press 4 three times or hold for 2 seconds.
- 2. Select **Options**. To do so, press \P or \blacktriangle and cofirm by pressing \clubsuit .
- 3. Select **Unlock**. To do so, press \P or $bar{f 1}$ and cofirm by pressing $bar{f 4}$.
 - » The display will now appear as shown in figure 63.
- » On delivery, the four-digit password is the device's serial number.
- 4. Inputting numbers:

Press and hold 1 to quickly scroll to the required number and either press it for 3 seconds or press to confirm the selected number (figure 64).





5. Moving back:

Press to switch to another input level. To move back, press

- 6. Confirm the four-digit password by pressing **IK**.
 - » The settings have been saved.

- » The °C/°F, BL On Time, Auto Off Time, Materialcalib., Password, Reset options are now activated.
- 7. Press 👫 to leave the **Options** menu.
- 8. Press 🔓 to leave the main menu.

9.5 Deactivating options

Once the device has been switched restarted, the °C/°F, BL On Time, Auto Off Time, Materialcalib., Password, Reset options will be deactivated again.

9.6 Selecting °C/°F

To do so: All of the options must be activated (see "9.4 Activating options").

- 1. Press three times or hold for 2 seconds.
- 2. Select **Options**. To do so, press \P or $\begin{center} \blacksquare \end{center}$ and cofirm by pressing $\begin{center} \blacksquare \end{center}$.
- 3. Select °C/°F. To do so, press ♥ or ▲ and cofirm by pressing ♣.
- 4. Navigate to the required temperature scale, i.e. Celsius (°C) or Fahrenheit (°F). To do so, press or $\stackrel{\bot}{\blacksquare}$ and confirm by pressing $\stackrel{\longleftarrow}{\blacksquare}$.
 - » The settings have been saved.
- 5. Press 4 to leave the **Options** menu.
- 6. Press **t** to leave the main menu.

9.7 Reducing the device's power consumption

9.7.1 Configuring the display illumination time

To do so: All of the options must be activated (see "9.4 Activating options").

- 1. Press \$\frac{1}{4}\$ three times or hold for 2 seconds.
- 2. Select **Options**. To do so, press \P or $dag{1}{4}$ and confirm by pressing $extstyle dag{4}$.
- 3. Select **BL On Time**. To do so, press **T** or **A** and confirm by pressing **4**.



- 4. Select the required display illumination period (30 seconds, 2 minutes, 5 minutes, 10 minutes). To do so, press or in and confirm by pressing.
 - » The settings have been saved.
- 5. Press 4 to leave the **Options** menu.
- 6. Press **t**o leave the main menu.

9.7.2 Configuring automatic switch-off

To do so: All of the options must be activated (see "9.4 Activating options").

- 1. Press three times or hold for 2 seconds.
- 2. Select **Options**. To do so, press \P or A and confirm by pressing \P .
- 3. Select **Auto Off Time**. To do so, press \P or $black ext{and confirm by pressing } black black ext{.}$
- 4. Select the period of time you want the device to stay switched on (3 minutes, 5 minutes, 10 minutes). To do so, press or in and cofirm by pressing.
 - » The settings have been saved.
- 5. Press 4 to leave the **Options** menu.
- 6. Press 🔓 to leave the main menu.

9.8 Configuring the material calibration function

The type calibration function is described in a separate operating manual.

9.9 Changing the password

To do so: All of the options must be activated (see "9.4 Activating options").

- 1. Press three times or hold for 2 seconds.
- 2. Select **Options**. To do so, press \P or \red and cofirm by pressing \red .
- 3. Select **Password**. To do so, press \P or $black ext{and cofirm by pressing } black black ext{.}$
 - » The display will show the current password.
- 4. Overwrite the current password. To do so, press and hold \(\bigcap_{\text{\cdots}} \begin{array}{c} 9 \text{ to quickly scroll to the required number and either press it for 3 seconds or press \(\bigcap_{\text{\cdots}} \bigcap_{\text{\cdots}} \end{array} \) to confirm the selected number.

Moving back:

Press to switch to another input level.


- 5. Confirm the new four-digit password by pressing **IK**.
 - » The setting has been saved.
- 6. Press to leave the **Options** menu.
- 7. Press **t**o leave the main menu.



9.10 Resetting the device to its factory settings

To do so: All of the options must be activated (see "9.4 Activating options").

- 1. Press 🙀 three times or hold for 2 seconds.
- 2. Select **Options**. To do so, press \P or $\begin{center} \blacksquare \end{center}$ and cofirm by pressing $\begin{center} \blacksquare \end{center}$.
- 3. Select **Reset**. To do so, press \P or $\stackrel{\bot}{\blacksquare}$ and cofirm by pressing $\stackrel{\longleftarrow}{\blacksquare}$.
 - » The display will then show the message Reset? (figure 65).
- 4. Confirm by pressing .
 - » The device will now be reset to its factory settings. All of your personal settings will be lost.
 - » The display will show the status indicator humi meter (figure 66).
 - » Resetting the device will not affect the saved measuring values.





10. Cleaning and maintenance

Regularly cleaning and maintaining the device will ensure that it will have a long service life and stay in good condition.

10.1 Changing batteries

The device constantly monitors the charge level of the batteries. The current battery status is shown on the status screen.

If the battery's charge is very low, the battery symbol will be shown with an exclamation mark. In that case, the batteries must be changed immediately (figure 68).

For changing the batteries, see section "3.3 Inserting batteries".





As the device's user, you are responsible by law for properly disposing of all used batteries, which must not be disposed of as domestic waste (Battery Directive).

5. Care instructions

- Do not leave the device out in the rain. The device is not waterproof.
- Do not expose the device to extreme temperatures.
- Protect the device from strong mechanical shocks and loads.

10.2 Cleaning the device

Plastic housing

• Clean the plastic housing with a dry cloth.

Measuring head

• The measuring head can be cleaned with a cloth and cleaning alcohol.



ATTENTION

Do not clean with fluids

Water or cleaning fluid getting inside the device can destroy the device.

▶ Only clean the plastic housing with dry materials.




11. Accessories

11.1 BLL tube extension

Optional accessory for extending the measuring tube one meter. Art.No. 12467

11.1.1 Overview tube extension and humimeter BLL

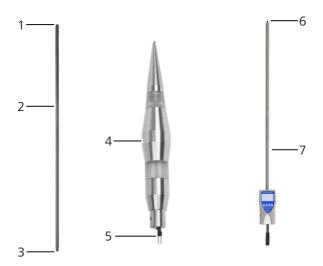

No	Name
1	Socket extension
2	Extension (tube)
3	Connenction extension
4	Measuring tip
5	Connection tip
6	Socket basic unit BLL
7	Basic unit BLL

11.1.2 Demounting of the measuring tip



CAUTION

Risk of injury

Risk of injury through the measuring tip.

- ► Keep the measuring tip away from your body during all activities.
- ► Keep the measuring tip away from other peoples' bodies during all activities.

Remove the batteries from the humimeter BLL.

Loosen the two screws which fix the measuring tip in the tube with a PH1 cross-head screwdriver.

Now carefully pull the tip out of the tube and release the connector between the tip and the tube.



11.1.3 Installation of the extension

Place the tube on the basic humimeter BLL unit together with the extension tube on a table.



Now insert the connector of the extension into the socket of the basic unit. (The socket can be held with tweezers, for example.) Make sure that the connector is pushed all the way into the socket.

Now carefully insert the extension tube into its basic unit tube.

Align the tube by twisting it, so the holes match up in order to apply the screws.

Now tighten the two M3x5 countersunk screws again.



11.1.4 Tip assembly

Carefully insert the plug of the measuring tip into the socket of the tube. (The socket can be held in place with tweezers, for example).



Now carefully insert the measuring tip into the tube. Now align the measuring tip by twisting it so that the holes match in order to attach the screws.

Now tighten the two M3x5 countersunk screws again.

11.1.5 Function test

Reinsert the batteries into the humimeter BLL.

Hold the measuring tip in the air: The measuring device must display a moisture value of 0.0.

Now grab the measuring tip with your hand: The measuring instrument must display a moisture value between 5 % and 50 %.

11.2 Changing the measuring head (tip)

If the measuring head is defective (e.g. the tip is broken), you can exchange it. For this purpose, the item: "Measuring head humimeter BLL (spare part)" Art.No. 12472 is required.

Please perform the steps described in item "11.1.2 Demounting of the measuring tip" page 44 and "11.1.4 Tip assembly" page 45. Then perform a functional test. See "11.1.5 Function test" page 45

12. Faults

If the measures listed below fail to remedy any faults or if the device has faults not listed here, please contact Schaller Messtechnik GmbH.

Fault	Cause	Remedy
Measuring error	The temperature of the material being measured is too low or high. I.e. the material's temperature is lower than 0 °C or higher than +40 °C	The temperature of the material being measured has to be between 0 °C and +40 °C.
	Temperature discrepancy between device and material being measured	Let the temperature adjust to the material being measured (permitted dif- ference of max. 3 °C).
	Wrong calibration curve	Check whether you have selected the right calibration curve (product) before taking a reading (see "6.3 Selection of calibration curve for wood chips").
	Moldy or rain wet wood chips	The accuracy of the measurement decreases significantly.
	Frozen wood chips or wood chips mixed with snow	The accuracy of the measurement decreases significantly.
	Water film on the measuring head	After measuring wet wood chips, on the measuring head may arise a water film. Clean the measuring head (see "10.2 Cleaning the device").
Data transfer to Log- Memorizer failed	Interface has not been configured	The interface only has to be configured once. To do so, press the F1 key on your computer and read the Help file for your Log- Memorizer program.



13. Storage and disposal

13.1 Storing the device

The device must be stored as follows:

- Do not store outdoors
- Store in a dry and dust-free place
- · Protect the device from sunlight
- Avoid mechanical shocks/loads
- Remove the batteries if the device isn't used for a period of 2 months or longer.
- Storage temperature: -20 °C to +60 °C

13.2 Disposing of the device



Devices marked with this symbol are subject to Directive 2012/19/ EU of the European Parliament and of the Council of 4 July 2012 on waste electrical and electronic equipment (WEEE).

If the device is being operated outside the European Union, the national regulations on the disposal of such devices that apply in the country of use must be observed.

Electronic devices must not be disposed of as domestic waste.

The device must be disposed of appropriately using appropriate collection systems.

14. Device information

14.1 CE declaration of conformity



Name/ Adresse des Herstellers: Schaller Messtechnik GmbH
Name/ address of manufacturer: Max-Schaller-Straße 99
A – 8181 St. Ruprecht

Produktbezeichnung: humimeter

Product designation:

Typenbezeichnung: BL2; BLL; BLH; BLW; FL1; FL2; FLH; FLM; FLS; RM1;

SLW: WLW

Type designation:

Produktbeschreibung: Messgerät zur Bestimmung des Wassergehalts in

Biomasse und diversen Schüttgütern

Product description Measuring device for determining the water content in bio-

mass and various bulk materials

Das bezeichnete Produkt erfüllt die Bestimmungen der Richtlinien:

The designated product is in conformity with the European directives:

EMV - Richtlinie 2014/30/EC EMC Directive 2014/30/EU
ROHS - Richtlinie 2011/65/EG RoHS-Directive 2011/65/EU

Die Übereinstimmung des bezeichneten Produktes mit den Bestimmungen der Richtlinien wird durch die vollständige Einhaltung folgender Normen nachgewiesen:

Full compliance with the standards listed below proves the conformity of the designated product with the provisions of the above-mentioned EC Directives:

EN 61326–1:2013 Elektrische Mess-, Steuer-, Regel- und Laborgeräte - EMV-An-

forderungen

Electrical equipment for measurement, control, and laboratory

use - EMC requirements

EN IEC 63000:2019-05 ersetzt / replaced EN 50581:2012 Technische Dokumentation zur Beurteilung von Elektro- und Elektronikgeräten hinsichtlich der Beschränkung gefährliche

Stoffe

Technical documentation for the assessment of electrical and electronic products with respect to the restriction of hazardous substances.



Für das angeführte Produkt ist eine vollständige Dokumentation mit Betriebsanleitung in Originalfassung vorhanden

For the mentioned product a complete documentation with manual of instruction in original version is available.

Bei Änderungen, die nicht vom Hersteller spezifiziert sind, verliert diese Konformitätserklärung die Gültigkeit.

In case of any changes not agreed upon with the manufacturer, this declaration of conformity loses its validity.

St. Ruprecht a.d. Raab, 31.07.2022

Mesechia / juminieter jom Schaller versich in Grübbl Acc - Singler (Machael 1998) AT-811 / Si Bohretter a. Rab www.bunizetecom | infoshynimetecom Bernhard Maunz Rechtsverbindliche | Interschrift des Ausstellers

Rechtsverbindliche Unterschrift des Ausstellers Legal binding signature of the issuer



DECLARATION OF CONFORMITY

Name/ address of manufacturer: Schaller Messtechnik GmbH

Max-Schaller-Straße 99 A – 8181 St. Ruprecht

Product designation: humimeter

Type designation: BL2; BLL; BLH; BLW; FL1; FL2; FLH; FLM; FLS; RM1;

SLW; WLW

Product description: Measuring device for determining the water content in bio

mass and various bulk materials

The designated product is in conformity with the following directives:

• Electromagnetic Compatibility Regulations 2016 Great Britain

 RoHS-Directive 2011/65/EU Directive on the restriction of the use of certain hazardous substances in electrical and electronic equipment

Full compliance with the standards listed below proves the conformity of the designated product with the provisions of the above-mentioned Directives:

EN 61326–1:2013 Electrical equipment for measurement, control, and laboratory

use - EMC requirements

EN IEC 63000:2019-05

replaced EN 50581:2012 Technical documentation for the assessment of electrical and electronic products with respect to the restriction of

hazardous substances.



For the mentioned product, a complete documentation with manual of instruction in original version is available.

In case of any changes not agreed upon with the manufacturer, this declaration of conformity loses its

St. Ruprecht a.d. Raab, 31.07.2022

Bernhard Maunz Legal binding signature of the issuer

14.2 Technical data

Display resolution	0.5 % moisture content, 0.5 °C/°F temperature
Measuring range	10 % to 50 % moisture content
Operating temperature	0 °C to +40 °C
Temperature measuring range	-10 °C to +80 °C
Storage temperature	-20 °C to +60 °C
Temperature compensation	Automatic
Data memory	Up to 10,000 measuring values
Power supply	4 x 1.5 Volt AA Alkaline batteries
Current consumption	60 mA (incl. display illumination)
Menu languages	German, English, French, Italian, Spanish, Portuguese, Czech, Polish, Russian, International
Display	128 x 64 illuminated matrix display
Device dimensions	1155 x 75 x 45 mm (without handle bar)
Device weight	830 g
Device IP rating	IP 40



15.	Notes			

h	ur	nir	ne	te	r B	LL	0	pe	rat	in	g N	Иa	nı	ıal																								
		•	•		-		•	•				-	-			•	•	•	-	-	•	•	٠	٠	•						-	-		-	•	•		
	٠			•		•	•	•	•	•	•	•	•	•	•	•	•	•			•	•						•		•	•	•	•	•	•			
٠	٠			•			•	•												٠	٠	•			•	•	•	•								٠	٠	
	•			•	•		•	•		•	•	•	•	•		•	•	•	•	•	•	•	•	•	•			•	•	•	•	•		•	•	•		
	٠	-	٠	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-	-	•	•	•	-	•		-	-	-	-	-	-	•	-	-	-	-	
								•								•	•											•		•						•		
٠				٠			٠	•														•						•										
												•	•										٠	٠		•	•						•	•			•	
•		٠			-							-	-								•		٠	٠	-	-	-		-		-	-		-				
									•	•	•	•	•															•		•	•	•						٠
												•	•	•												٠	٠		٠		•	•		•				
•																																						



							٠					٠			٠	•	•					٠			•			•		•	•	•	•				•	
•	•	•	•	•	•	•	•	•	•	•	•	•	•	•	•	•	٠	٠	٠	٠	•	•	•	•	•	•	•	•	•	•	•	•	•	•	•	•	•	•
٠	٠						•	•	•		•	•	•		٠	٠		٠	٠	٠										•	•							٠
			•				-					-		-		-	•					•								-	-	-	-					
																																•	•			•	•	•
٠	٠	•	•	•	•	•	•		•	•	•	•			٠	•	•	٠	٠	٠	٠			•	•	•	•	•	•		•	•	•	•	•	•		٠
												_																										
•				•			٠	•	•	•	•	•	٠	•	٠	٠	٠	٠						•	•	•	•	•	•	•	•	•	•	•	•	•	•	•
																														•	•	•						
		٠	٠	٠	٠	٠	٠	٠	٠	٠	٠				٠	٠	٠			٠		٠	٠	٠	٠	٠											٠	٠













Schaller Messtechnik develops, produces and sells professional moisture meters and turnkey solutions.

Schaller Messtechnik GmbH

Max-Schaller-Straße 99, A - 8181 St. Ruprecht an der Raab Tel +43 (0)3178 - 28899, Fax +43 (0)3178 - 28899 - 901 info@humimeter.com, www.humimeter.com